

Al-Mustaqbal University.
College of Engineering and Technologies.
Biomedical Engineering Department.

Subject: Biomedical Instrumentation Design_II.

Class (code): 5th (MU0115202).

Lecture: 4 and 5




BMID_II

1

Data Acquisition, Part 1

BMID_II

- › No is the production of the x-ray that travels through 3D space (the example below shows 10 voxels)
- › Depending of the amount of density encounters (air, liquid, and/or bone) there will be a variation in the ray's attenuation. These values of attenuation is referred to as μ_i where the beam may encounter different degrees of attenuation within a certain volume of voxels. The end point of the attenuated ray is then referred to N_i were the detector records the amount of attenuation. End results - linear attenuation coefficient, μ , that occurs from that specific x-ray

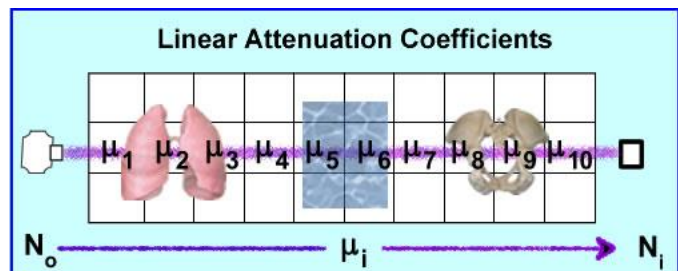

2

Data Acquisition, Part 1

BME 525

- > The chart shows attenuation coefficients for a 100 kVp x-ray beam. While a CT tube uses a poly-energetic beam within 100 kVp (1% variation), its output can be adjusted between 70 and 140 kVp.
- > The attenuated sum (X_n) occurs after the initial ray N_o passes through a set of voxels, which in turn becomes N_i and can be written as $X_i = -\ln(N_i/N_o)$.
- > When a narrow beam of mono-energetic photons with an incident intensity I_o , penetrating a layer of material with mass thickness x and density ρ , emerges with intensity I given by the exponential attenuation law as:

$$I = I_o \exp \left[- \left(\frac{\mu}{\rho} \right) x \right]$$



Linear Attenuation Coefficients (cm ⁻¹)	
Bone	0.528
Muscle	0.237
Brain White	0.213
Brain Gray	0.212
Blood	0.208
Water	0.206
Fat	0.185
Lung	0.093
Air	0.0004

3

Data Acquisition, Part 1

BME 525

- > How CT actually determines the μ value in a voxel?
- > Consider look at a 2x2 matrix using an iterative algorithmic approach, Algebraic Reconstruction Technique (ART).
- > The attenuation in these 4 pixels are hypothetically unknown, however, when applying an x-ray beam to them, N_o , at six different angles, 6 N_i , the values are detected (N_{1-6}). This is demonstrated below

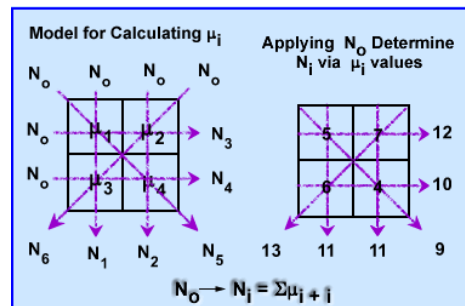

4

π

Algebraic Reconstruction Technique (ART)

- › A low-complexity iterative solver to the algebraic reconstruction problem
- › Starts with an initial estimate and tries to push the estimate closer to the true solution
 - Instead of back-projecting the average ray value, the error between the projection computed from current estimate and the true is used

$$Update = (P_{\theta}(\rho) - \sum_{x,y} \alpha_{\rho}^{\theta}(x,y) \cdot \hat{I}(x,y)) / N$$




Update = (True Projection - Estimated Projection) divided over all points in projection path

5

 π

ART Example

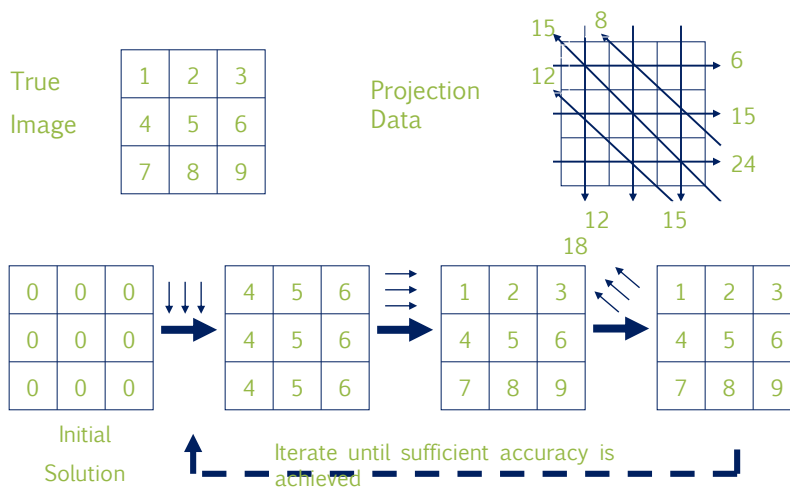

6

Data Acquisition, Part 1


BME
525

- › All makes, and models of CT scanners are similar in that they consist of a scanning gantry, x-ray generator, computer system, operator's console, and physician's viewing console.
- › CT can be broken down into three segments: data acquisition, image reconstruction, and image display.
- › Data are acquired when x-rays pass through a patient to strike a detector and are recorded. The major components involved in this image creation phase are the gantry and the patient table.

7


BME
525

- › The gantry is the ring-shaped part that houses many of the components necessary to produce and detect x-rays.
- › The range of gantry aperture size is typically 70 to 90cm, and can be tilted either forward or backward (usually $\pm 15^\circ$ to $\pm 30^\circ$) as needed to accommodate a variety of patients and examination protocols.
- › The gantry also includes a laser light that is used to position the patient within the scanner.

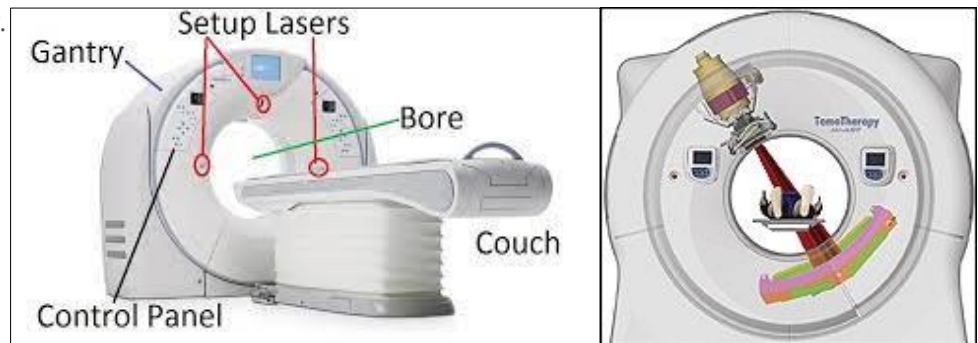


8


BME
525

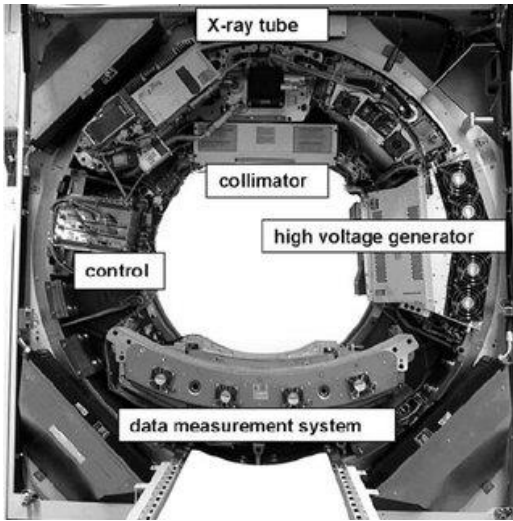

9

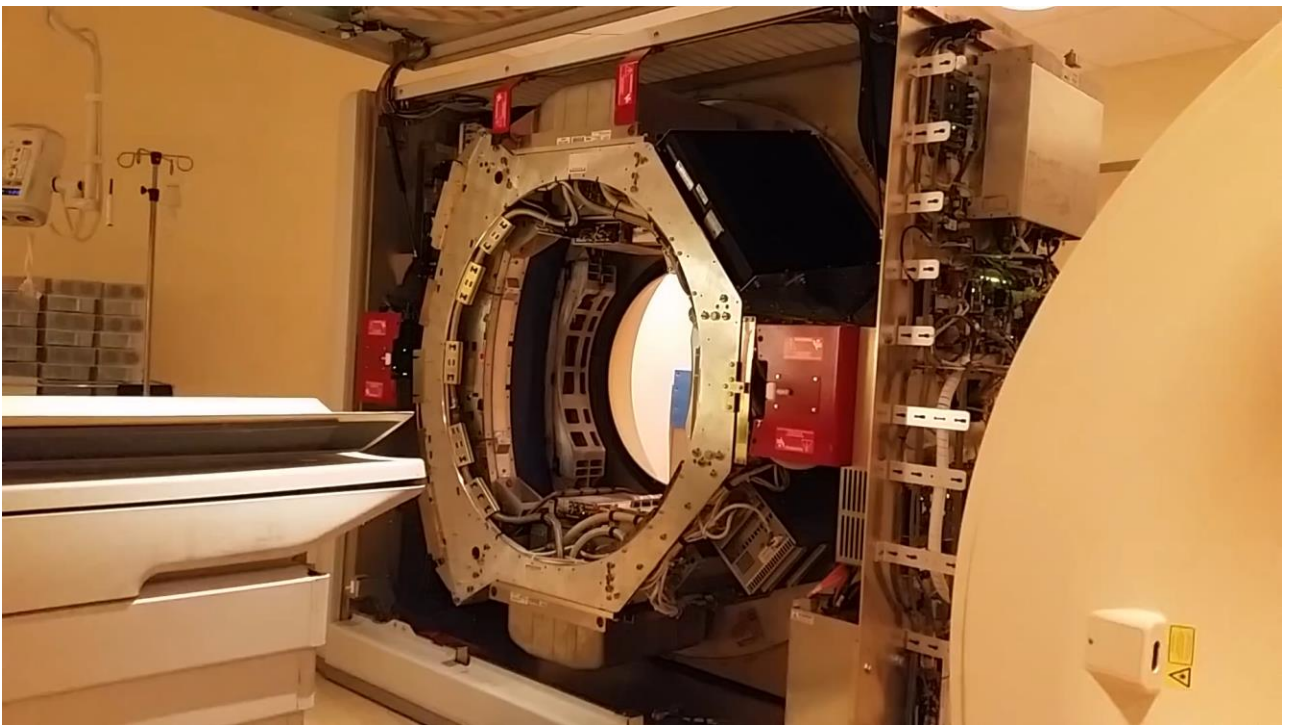


10

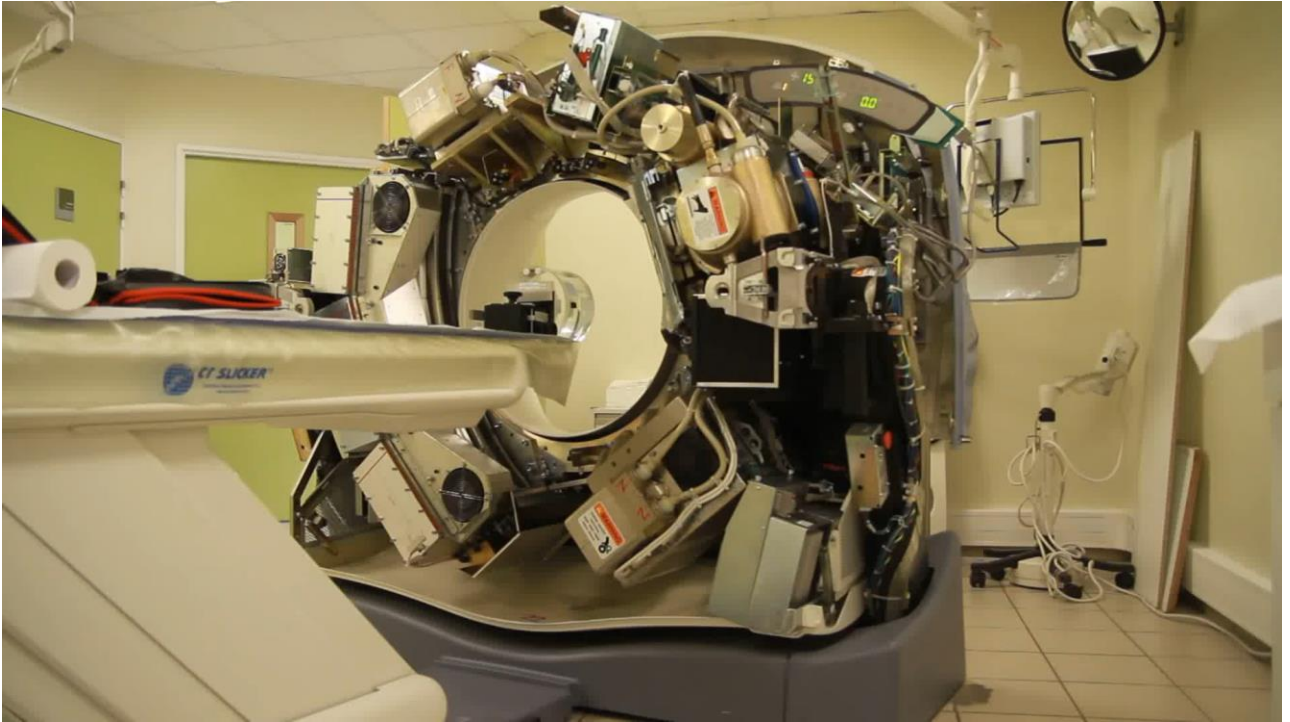

11


- › Slip rings are electromechanical devices that use a brush-like apparatus to provide continuous electrical power and electronic communication across a rotating surface.
- › They permit the gantry frame to rotate continuously, eliminating the need to straighten twisted system cables.
- › Slip rings used to bring power to x-ray tube on rotating gantry of a helical CT machine and, for some designs, to acquire information from the detector array.

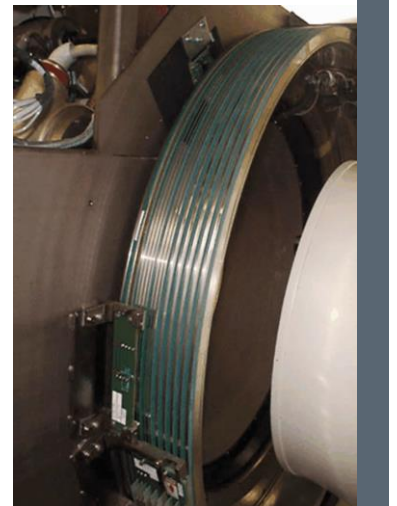

12

BME
525

- › The shiny metal strips carry electric signals that are swept off by special brushes. The brushes are not in the form of bristles but rather of metal blocks (in this case a silver alloy).
- › The five pairs of larger brushes provide the voltage required by the x-ray tube, and the three pairs of smaller ones transfer signals from the gantry controller.

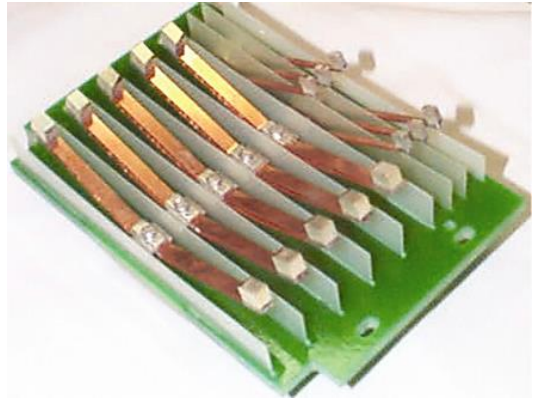

13

14

BME
525

- › *High-frequency generators* can be located within the gantry.
- › Generators produce high voltage and transmit it to the x-ray tube. The power capacity of the generator is listed in kilowatts (kW), and determines the range of exposure techniques (i.e., kV and mA settings) available on a particular system.
- › CT generators produce high kV (generally 120–140 kV) to increase the intensity of the beam, which will increase the penetrating ability of the x-ray beam and thereby reduce patient dose.
- › In addition, a higher kV setting will help to reduce the heat load on the x-ray tube by allowing a lower mA setting. Reducing the heat load on the x-ray tube will extend the life of the tube



15



BME
525

- › The CT tube is designed to handle the stresses of the scanning protocols that often require multiple long exposures performed on numerous patients daily.
- › The way a tube dissipates the heat that is created during x-ray production is critical.
- › All manufacturers list generator and tube cooling capabilities in their product specifications.
 - KW: the system generator's maximum power in KW.
 - MHU: the anode heat capacity in million heat units (MHU), e.g. 7 MHU tube will last more than 150 million mAs.
 - KHU: the maximum anode heat dissipation rate in thousand heat units (KHU).
- › These specifications can be helpful in comparing various CT systems. Also it is important to compare the length of protocols that the tube will allow and how quickly they can be repeated.

16

BME
525


- › Collimators restrict the x-ray beam to a specific area, thereby reducing scatter radiation.
- › Scatter radiation reduces image quality and increases the radiation dose to the patient.
- › Reducing the scatter improves contrast resolution and decreases patient dose.
- › Collimators control the slice thickness by narrowing or widening the x-ray beam. The source collimator is located near the x-ray source and limits the amount of x-ray emerging to thin ribbons.

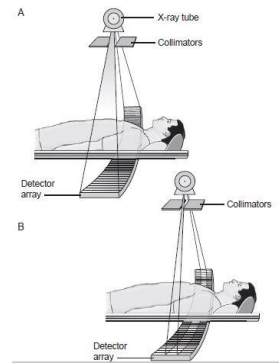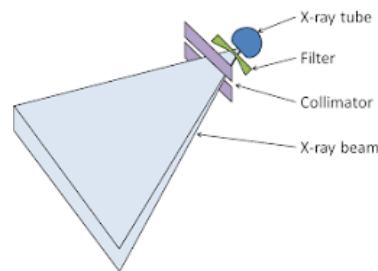

17

BME
525


- › The source collimator affects patient dose and determines how the dose is distributed across the slice thickness (i.e., dose profile).
- › The source collimator resembles small shutters with an opening that adjusts, dependent on the operator's selection of slice thickness.
- › In MDCT systems (Multidetector computed tomography), slice thickness (0.5 to 10 mm) is also influenced by the detector element configuration.

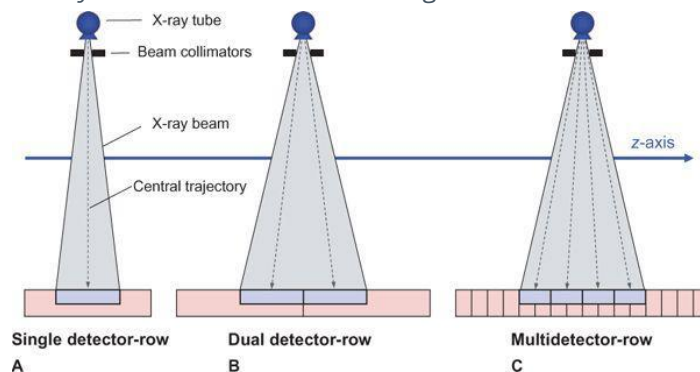

18

BME
525


- › Some CT systems also use pre-detector collimation located below the patient and above the detector array.
- › This collimator shapes the beam after it has passed through the patient.
- › The primary functions of pre-detector collimators are to ensure the beam is the proper width as it enters the detector and to prevent scatter radiation from reaching the detector.

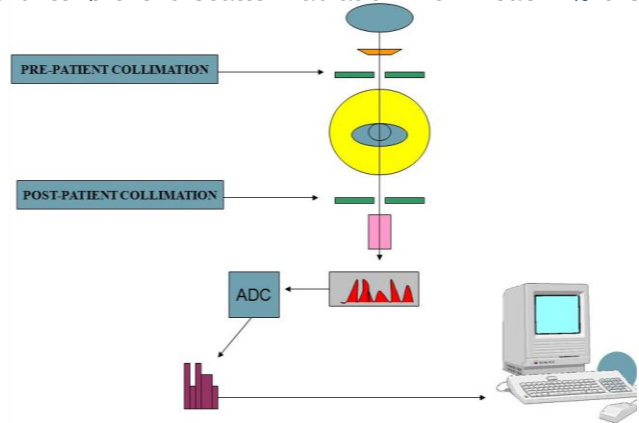

19

BME
525


- › The detectors collect information regarding the degree to which each anatomic structure attenuated the beam while passing through the patient.
- › The detector array comprises detector elements situated in an arc or a ring, each of which measures the intensity of transmitted x-ray radiation along a beam projected from the x-ray source to that particular detector element.

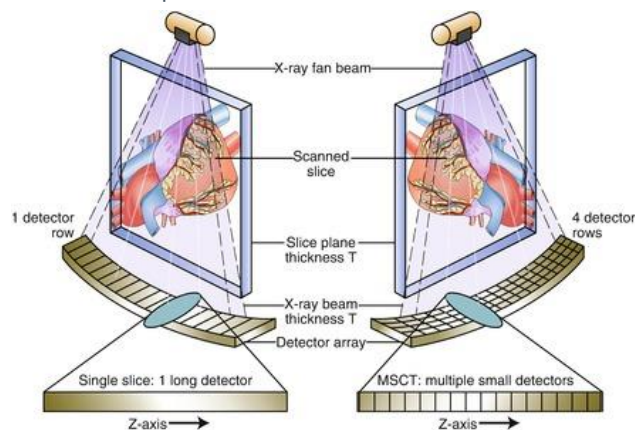

20

BME
525

- › Also included in the array are elements referred to as reference detectors that help to calibrate data and reduce artifacts.
- › The scan field of view determines the size of the fan beam, which, in turn, determines the number of detector elements that collect data.
- › Detectors can be made from different substances, each with their own advantages and disadvantages

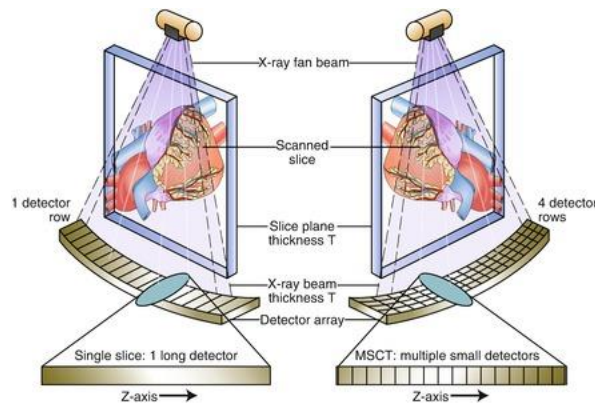

21

BME
525

- › *The optimal characteristics of a detector are as follows:*
- › 1) high detector efficiency, defined as the ability of the detector to capture transmitted photons and change them to electronic signals;
- › 2) low, or no, afterglow, defined as a brief, persistent flash of scintillation that must be taken into account and subtracted before image reconstruction;
- › 3) high scatter suppression;
- › 4) high stability, which allows a system to be used without the interruption of frequent calibration.

22

BME
525

- › Overall detector efficiency is the product of a number of factors. These are 1) stopping power of the detector material;
- › 2) scintillator efficiency (in solid-state types);
- › 3) charge collection efficiency (in xenon types);
- › 4) geometric efficiency, defined as the amount of space occupied by the detector collimator plates relative to the surface area of the detector;
- › 5) scatter rejection.

23

BME
525


- › Capture efficiency: the ability with which the detector obtains photons that have passed through the patient.
- › Absorption efficiency: the number of photons absorbed by the detector and is dependent on the physical properties of the detector face (e.g., thickness, material).
- › Response time: is the time required for the signal from the detector to return to zero after stimulation of the detector by x-ray radiation so that it is ready to detect another x-ray event.
- › The detector response is generally a function of the detector design.
- › Dynamic range: is the ratio of the maximum signal measured to the minimum signal the detectors can measure.

24

- › All new scanners possess detectors of the solid-state crystal variety.
- › Detectors made from xenon gas have been manufactured but have largely become obsolete as their design prevents them from use in MDCT systems.
- › However, some xenon gas detector systems may still be in use on older models.

TABLE 2-1 Characteristics of Detectors

Solid-State Crystal	Pressurized Xenon Gas
High photon absorption	Moderate photon absorption
Sensitive to temperature, moisture	Highly stable
Solid material	Low-density material (gas)
Can exhibit afterglow	No afterglow
No front window loss	Losses attributable to front window and the spaces taken up by the plates


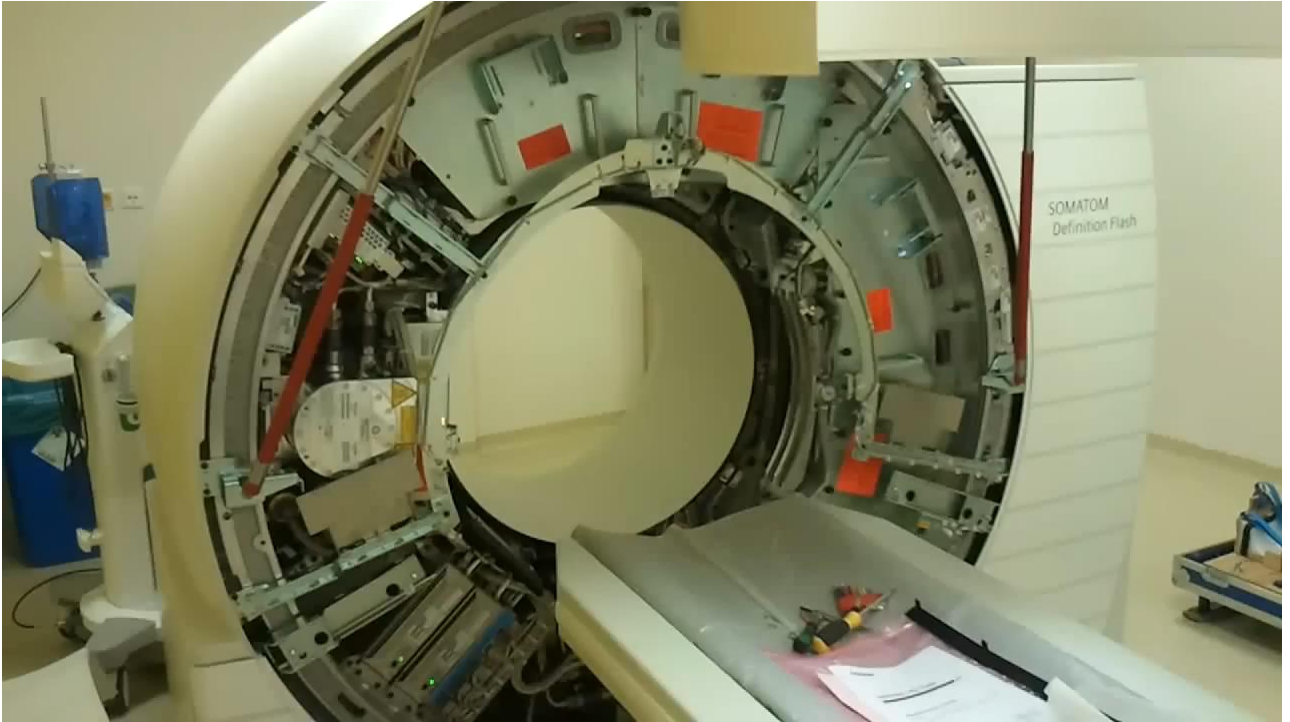


27

Data Acquisition, Part 2

BME
525


- › Third-generation CT scanner.
- › Reference detectors are typically located at either end of the detector array to measure the unattenuated x-ray beam.
- › The rotating detector design allows all of the readings that make up a view to be recorded instantaneously and simultaneously >>> thus reducing scan times and patient motion artifacts. resulting from patient motion.
- › An advantage of the third-generation system is that the tube is directly focused on the detector array.

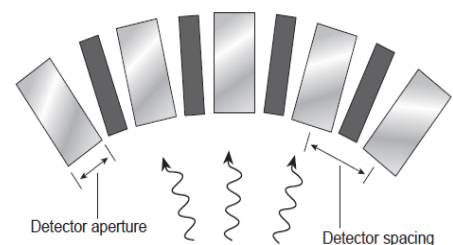

28

BME
525

- › A disadvantage of the third-generation design is the more frequent occurrence of ring artifacts. Because the same bank of detectors is used repeatedly, *even a very small misalignment of a single detector will result in a visible ring artifact.*

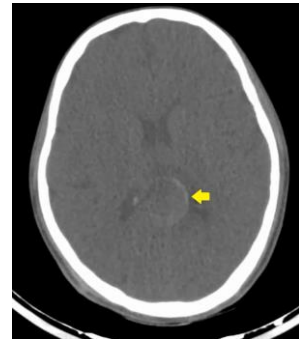


29

BME
525

- › *Detector Electronics*
- › X-ray photons that strike the detector must be measured, converted to a digital signal, and sent to the computer.
- › This is accomplished by the data-acquisition system (DAS), which is positioned within the gantry near the detectors.
- › Signals emitted from the detectors are analogue (electric), whereas computers require digital signals. Therefore, one of the tasks of the DAS is to convert the analog signal to a digital format.
- › To measure the x-ray photons that have penetrated the patient, the DAS samples the detectors as many as 1,000 times per second.

30

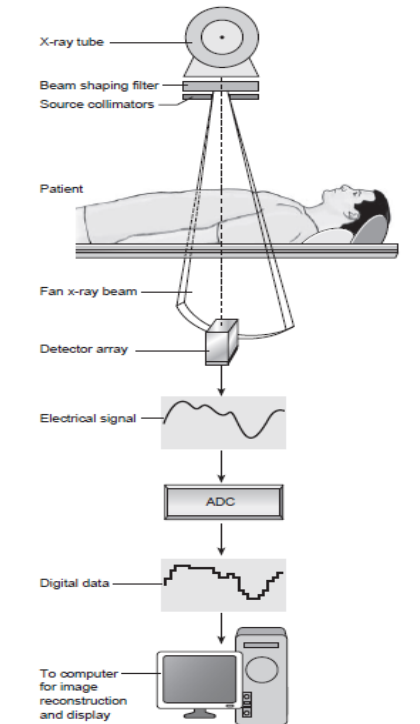
BME
525

31

BME
525

› *Patient table*

- › The patient lies on the table (or couch) and is moved within the gantry for scanning.
- › The process of moving the table by a specified measure is most commonly called incrementation, feed, step, or index.
- › Helical CT table incrementation is quantified in millimeters per second because the table continues to move throughout the scan.
- › The degree to which a table can move horizontally is called the scannable range, and will determine the extent a patient can be scanned without repositioning.

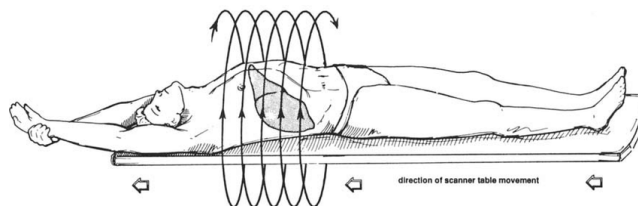

32

CT GANTRY CONTROL PANEL

1. Gantry Tilt (+/-30 degrees).
2. Laser Alignment Lights on/off.
3. Couch in/out.
4. Free (manual) Couch Movement.
5. Zero Couch Position.
6. Couch up/down.
7. Home Button (couch out & down).




33

› *Dual Energy CT (DECT)*

- › Dual-energy CT, also known as spectral CT, is a computed tomography technique that uses two separate x-ray photon energy spectra, allowing the interrogation of materials that have different attenuation properties at different energies.
- › Whereas conventional single-energy CT produces a single image set, dual-energy data (attenuation values at two energy spectra) can be used to reconstruct numerous image types:
 - › Weighted average images (simulating single energy spectra).
 - › Virtual monoenergetic images (attenuation at a single photon energy rather than a spectrum).

34

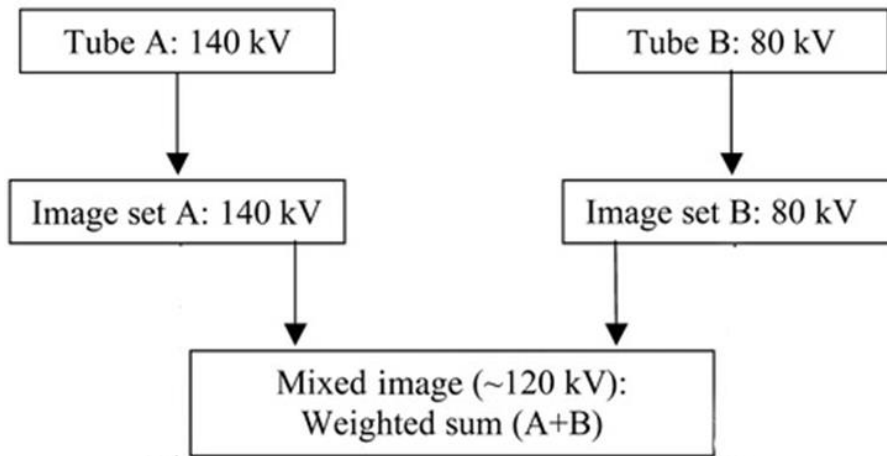

35

- › **material decomposition images:** is a method for differentiation and quantification of materials in a sample and it utilizes the energy dependence of the linear attenuation coefficient, i.e. mapping or removing substances of known attenuation characteristics, such as iodine, calcium, or uric acid):
- › virtual non-contrast images (iodine removed).
- › Iodine concentration (iodine maps): used to detect pulmonary embolism (PE) with CT angiography.
- › Calcium suppression (calcium removed (CaSupp)): used to observe bone marrow edema by removing calcium components from the image.
- › Uric acid suppression (uric acid removed): used for the diagnosis of gout. It is a good noninvasive alternative to synovial fluid aspiration.

36